

MRO FTT/NAS & FLC ICD


FTT/NAS to ISS ICD

MRO-ICD-CAM-1100-0112

The Cambridge FTT Team

rev 1.21

22 August 2017

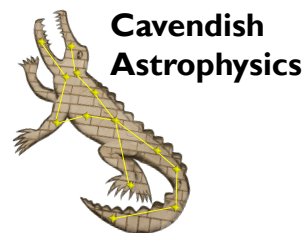

Cavendish Laboratory
JJ Thomson Avenue
Cambridge CB3 0HE
UK

ICD Description

Specific entry from the ICD N² Table contained in FDR document.

ICD Number	Sub-systems	Org	Owner	Brief description and preliminary contents
MRO-ICD-CAM-1100-0112	FTT-NAS	MRAO	JSY	Interface between FTT/NAS control software and ISS, based on the Generic System Interface framework

Change Record

Revision	Date	Author(s)	Changes
0.1	2012-04-30	EBS	First draft version
0.2	2012-05-01	EBS/JSY/MF	Complete rewrite
0.3	2012-05-02	EBS/JSY/MF	Changes to subscriptions
1.0	2013-12-18	JSY	Update for first software release
1.1	2014-01-10	JSY	Added notes on implementation of variants. Minor corrections
1.2	2014-05-22	JSY	Added boolean system properties (were omitted in error). Added new system properties, monitor points and commands for Kalman filter, removed placeholder servo parameters. Added fault names
1.3	2014-06-04	JSY	Added AuxTip, AuxTilt, AllowAuxTipTiltIn (FTT only)
1.4	2014-11-27	JSY	Added OpticalGainX, OpticalGainY, setTipTiltServoGain, TipTiltServoGain, AvgCentroidErr
1.5	2015-03-02	JSY	Changes for frame-type-specific background images: new/removed system properties e.g. DarkFullExpTime; modified commands e.g. getDarkFrame; new/removed monitor points e.g. DarkFullFrameSet. Added CameraAirCooling (implemented May 2014)
1.6	2015-03-19	JSY	Added CCDSetTemp. Removed CICScaling system property, useCICModel and ignoreCICModel commands, and CICModelUsed monitor point
1.7	2015-05-20	JSY	Removed getTipTiltServoParams (implementation removed May 2014). Removed UseIOCard, UseCamera, CameraAirCooling, AllowCustomReadout monitor points (no need to implement in GSI interface as they directly correspond to system properties). Added getter commands for unit tests
1.8	2015-06-04	JSY	Added startUcamControl/Display commands and port number system properties for the dlmsg interface
1.9	2015-06-08	JSY	Added commands and status item for control of air flow
1.10	2015-06-10	EBS	Removed getter commands. Changed ForceShutdown monitor point to CameraEnable, removed HeaterPower. Replaced obsolete setHeatPower command with setHeatOn and setHeatOff. Added LabJack fixed parameters. Added AirFlowTooLow fault constraints.

1.11	2015-06-25	EBS	Minor edit to track software name changes.
1.12	2015-06-30	JSY	Additional environment controller monitor points (implemented some time ago)
1.13	2015-11-13	EBS	Track environment controller's new ability to shut down camera controller.
1.14	2016-02-23	JSY	Additional system properties, monitor points and faults related to shutdown/power outlet control.
1.15	2017-02-09	EBS	Added temperature and humidity calibration parameters for environment controller.
1.16	2017-05-31	EBS	Added new publish and subscribe commands, changed power board fixed parameters.
1.17	2017-06-16	EBS	Changed LabJack interface names. Removed HeaterPower. Added airflow valve fault.
1.18	2017-06-26	EBS	Track hardware changes to environmental controller fixed parameters and monitor points.
1.19	2017-06-26	EBS	Fixed uncapitalised environmental controller monitor point names.
1.20	2017-07-12	EBS	Track changes to environmental controller monitor point ordering.
1.21	2017-08-22	JSY	Added flow rate calibration parameters for environment controller.

Notification List

The following people should be notified by email that a new version of this document has been issued:

MROI: Allen Farris
Andres Olivares

MRAO: Chris Haniff
John Young
David Busher
Martin Fisher

Table of Contents

1	Introduction	5
2	Requirements	6
3	Design	7
3.1	System variants	9
3.1.1	C Implementation	10
4	Interface Control	11
4.1	System controller interface	11
4.1.1	System properties.	11
4.1.2	Control	14
4.1.3	Monitor points	18
4.1.4	Subscriptions	22
4.1.5	Faults	23
4.2	Environment controller interface	23
4.2.1	System properties.	23
4.2.2	Control	26
4.2.3	Monitor points	27
4.2.4	Subscriptions	28
4.2.5	Faults	28

Scope

This document describes the software interfaces of the FTT/NAS to the ISS. These comprise the Generic System Interface and the additional network requirements of the software. Interfaces internal to the FTT/NAS software and hardware interfaces required by the software are not described.

Acronyms and Abbreviations

API	Applications Programming Interface	MROI	Magdalena Ridge Observatory Interferometer
CSV	Comma Separated Values	NAS	Narrow-field Acquisition System
FLC	First Light Camera	NMT	New Mexico Tech
FTT	Fast Tip-Tilt	NTP	Network Time Protocol
FTTA	Fast Tip-Tilt Actuator	TBC	To be confirmed
GSI	Generic System Interface	TBD	To be determined
GUI	Graphical User Interface	UT	Unit Telescope
ISS	Interferometer Supervisory System	UTCS	Unit Telescope (Mount) Control System
MMCDB	MROI Monitor and Configuration DataBase	UTM	Unit Telescope Mount

Documents

Drawings

Reference Documents

- RD1** Technical Requirements: Fast Tip-Tilt/Narrow-field Acquisition System (INT-403-ENG-0003) – rev 2.2, May 20th 2010
- RD2** Technical Requirements: First Light Camera (INT-403-TSP-0107) – rev 1.0, May 20th 2010
- RD3** Interface spreadsheet for FTTCamSystem – <http://www.mrao.cam.ac.uk/research/OAS/pmwiki/uploads/MROI FastTipTilt.InterfaceControl/FTTNAS-ISS-Spreadsheets.tar.gz>
- RD4** Interface spreadsheet for FTTEnvSystem – <http://www.mrao.cam.ac.uk/research/OAS/pmwiki/uploads/MROI FastTipTilt.InterfaceControl/FTTNAS-ISS-Spreadsheets.tar.gz>
- RD5** UTCS Design Description (MRO-TRE-OSL-6100-004) – issue 15
- RD6** The UTCS to ICS Interface (MRO-TRE-OSL-6100-007) – issue 15

Applicable Documents

- AD1** Interface to an MROI System INT-409-ENG-0020 – version 1.5, January 31st 2013

1 Introduction

This ICD, in conjunction with the interface spreadsheets RD3 and RD4, defines the interfaces between the FTT/NAS control software and the MROI Interferometer Supervisory System (ISS).

A separate ICD describes the interfaces between the FLC and the ISS. However, it is important to understand that FLC and FTT/NAS software are not separate implementations (except that there are separate FLC and FTT/NAS editions of the control GUI). Rather there is a single software package, for which a well-defined subset of the functionality satisfies the FLC technical requirements (RD2). The FLC subset has been implemented and tested first, and so the FLC ICD defines the more mature fraction of the functionality (system properties, commands, and monitor points). This subset includes all of the functionality needed to commission the Unit Telescope.

The single implementation has been designed to work with either the FLC or FTT/NAS hardware, with appropriate changes to the values of the system properties.

The ISS is responsible for coordinating the actions of the many quasi-autonomous systems that comprise the interferometer control system. In particular, the ISS is responsible for:

- Starting and configuring the systems;
- Sequencing and coordinating the actions of multiple systems in order to collect science data efficiently;
- Collecting monitor data and storing it in a central database;
- Managing faults and error conditions;
- Shutting down the systems in an orderly fashion at the end of observing (where applicable).

The ISS consists of several components which function in concert to provide supervisory control of the interferometer:

Database Manager Mediates access to the central MROI Monitor and Configuration Database (MMCDB).

Executive Starts and configures the systems. Configuration parameters are obtained from the MMCDB.

Supervisor Commands the systems once they have been initialized.

Data Collector A distributed system of Data Collectors collect monitor data published by the systems and import the data into the MMCDB.

Publish-Subscribe System A service provided by the Database Manager and Data Collectors that allows any system to subscribe to specific monitor data published by any other interferometer systems.

Fault Manager Responds to fault notifications published by systems.

When the various ISS components need to communicate with individual interferometer systems, they do so through a network interface which uses a custom communications protocol over TCP/IP sockets. Systems implement the server side of this communications link, and can accept connections from multiple remote clients. Clients can send commands and receive responses by connecting to one TCP port, and receive monitor data and the results of long-running commands by connecting to another port. Code for encoding and decoding network messages on both sides of this interface is generated from spreadsheets that define the particular commands and monitor variables that each kind of system implements, as well

as the types of fault that can be generated. The code-generation framework, known as the Generic System Interface (GSI), is supplied by MRO. There are versions of the GSI that generate Java and C code.

As agreed with MRO, we use different variants of each interface spreadsheet to suit the various deployment scenarios. These are outlined in Sec. 3.1 below. To keep the total number of spreadsheets manageable, there is no separate FLC interface spreadsheet (this is a change from the approach suggested at PDR). Instead, the accompanying spreadsheets define all of the commands and monitor points anticipated for the final FTT/NAS software implementation. For convenience, the FLC ICD lists only the subset that satisfies the FLC requirements. The other commands and monitor points are implemented such that they can be executed/published, however in early releases their functionality may be limited.

Thus the steps needed to interface a system (or collection of related systems) to the ISS are:

- Create a spreadsheet based on an MRO-supplied template that defines:
 - The system classes;
 - The commands that instances of each class accept, their parameters, and whether they should run in a separate thread (such commands are called “asynchronous” commands);
 - The monitor points that instances of each class publish and their data types;
 - The types of fault that may be published.
- Write a suitable `main()` function that initializes the network interface.
- Write custom state change actions that will be executed during transitions between states of the standard model for GSI-based systems (for example actions to initialize and shut down the system).
- Write custom methods that implement the commands defined in the spreadsheet.
- Optionally, write custom getter methods that return new values of the monitor points defined in the spreadsheet (these are only needed if the monitor points are to be polled at intervals initially defined by the spreadsheet and adjustable by the client; otherwise systems may publish monitor data at times of their choosing using generated publish methods).
- Run the GSI code generation tool on the spreadsheet to generate code that encodes or decodes network messages corresponding to the defined commands and monitor points.
- Compile the custom methods and link these against the generated code and a static code library.
- The result will be an executable that implements the network interfaces to the ISS and calls the appropriate custom code to actually execute commands and get monitor points.

This ICD accompanies the six interface spreadsheets (three variants of each of two systems) in order to provide some additional context for the definitions they contain.

Besides providing the network interface, the GSI also provides a standalone execution environment, in which commands may be executed from a script or by calling their C methods directly, rather than being sent from a remote client. The direct method call approach allows any command to be executed whereas the scripting implementation does not support all of the possible datatypes.

2 Requirements

Many of the top-level requirements that apply to the FTT/NAS (RD1) will only be satisfied if the control software operates correctly. The MROI Generic System Interface is an integral part of that control

software, even when it is being used in standalone mode with no network connection to the ISS.

The network interface to the ISS is required to realize the target acquisition and fast tip-tilt correction functionality, as telescope steering corrections/offloads are sent to the Unit Telescope Mount's control system (UTCS) via the ISS (this design choice was at MRO's request), and certain information published by the UTCS that is needed by the FTT/NAS will be obtained via the ISS Publish-Subscribe System (PSS).

The FTT/NAS software requires the following interfaces external to the FTT/NAS hardware:

- Ethernet network support (100BASE-T or faster), for communication with the ISS and between the software components. However, the software can also work in stand-alone mode, where all the components run on one computer.
- A network interface to the ISS, based on the GSI framework outlined above. This enables the FTT/NAS to communicate with the ISS (and the local UTM) over the network using the GSI. The software makes use of the following GSI facilities:
 - Control.
 - Monitor point publishing.
 - Error and exception handling.
 - The publish/subscribe system. Necessary for telescope communication.
- An external networked computer running Linux, for the control GUI.
- An external networked computer for the analysis GUI. The preliminary analysis GUI requires an installation of Python.
- A Network Time Protocol (NTP) server running on the local network, for accurate timestamping of FTT/NAS data.

3 Design

The software consists of four independent components (Figure 1):

1. The system controller is responsible for controlling the fast tip-tilt camera and using camera data to perform source image acquisition and stabilisation.
2. The environment controller is responsible for maintaining a thermally safe camera environment and collecting environmental FTT/NAS data.
3. The control GUI permits interactive control, monitoring, and logging of data from the system controller and the environment controller when equivalent ISS facilities are not available or not convenient. There are distinct FLC and FTT/NAS editions of the control GUI. The FLC edition has a simpler user interface and can log image centroids to CSV files, as requested by AMOS, as well as FITS.
4. The analysis GUI analyses and graphs data logged by the control GUI.

The system controller and the environment controller communicate with the ISS over the network using the GSI protocol. They also communicate with the control GUI over the network using the dlmsg protocol, a messaging system developed by Cambridge.

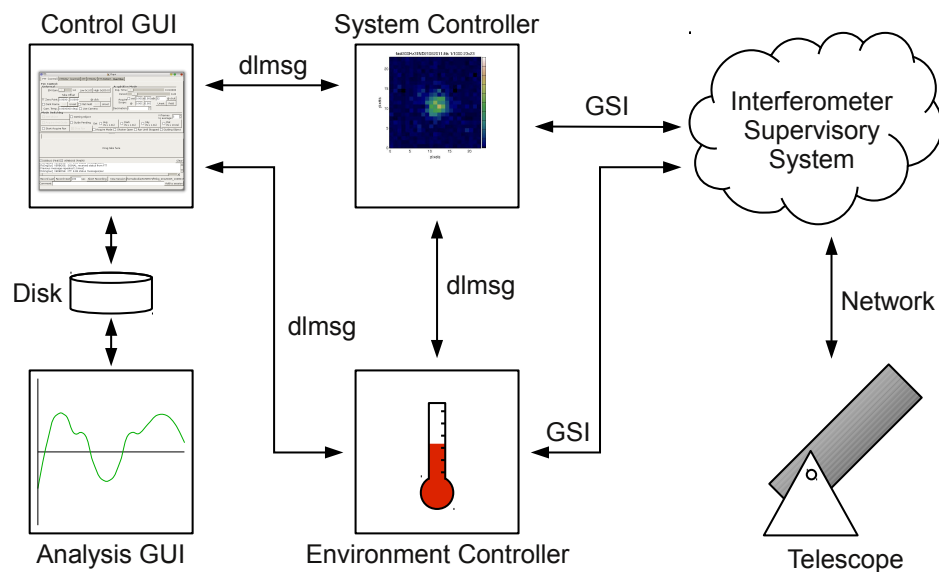


Figure 1: ISS-centric overview of the FTT/NAS software.

The control GUI logs and saves data generated by the system controller, the environment controller and itself. These data can be analysed later by the analysis GUI.

The network requirements depend on how the FTT/NAS software is deployed. The system is designed to be very flexible in this respect. Some possible scenarios are:

- The four components all run on the FTT/NAS computer and communicate via loopback interfaces. In this case, no network is required, this is a complete standalone system, however telescope communication will not be available.
- The environment controller runs on an independently powered embedded processor while the other components run on the FTT/NAS computer. This may be regarded as the minimum “safe” configuration as it provides awareness of the environment even when the FTT camera is completely powered down. If both computers are located within the control rack, this scenario only requires network functionality within that rack.
- The system controller runs on the FTT/NAS computer, the environment controller runs on the embedded processor, and the control GUI and analysis GUI run remotely, for example on a laptop computer in the telescope enclosure or in the interferometer control room. This requires an operational network but no networked GSI interface is required.
- The system controller runs on the FTT/NAS computer, the environment controller runs on the embedded processor, and the control GUI and analysis GUI run remotely. The ISS also has access to the controllers via the GSI. Depending on the configuration, either the control GUI or the ISS has control of the system, the other can only monitor the system and issue commands that do not

change the system state.

- The system controller runs on the FTT/NAS computer, the environment controller runs on the embedded processor, and they both communicate with the ISS via the networked GSI. The control and analysis GUIs are not needed. This is the expected final configuration of the system.

The system controller also needs to communicate with the local telescope to send steering corrections and receive the current rotation matrices and (if applicable) guide target offsets. This communication relies on availability of the GSI publish-subscribe system.

3.1 System variants

The software comprises several variants of each of the system controller and environment controller, for use in the deployment scenarios outlined above and for testing the system. Each variant:

- has a unique executable whose name follows the convention outlined below;
- uses one of several interface spreadsheets to define the accepted commands;
- implements the network interfaces to the control GUI only if needed for the intended deployment scenario(s).

Matching filenames are used for the executable and interface spreadsheet, comprising the components outlined below.

1. A prefix indicating the role of the executable (the same spreadsheet is used irrespective of the executable prefix).

utest_ Executes a unit test suite.

test_ Executes a standalone test script.

start_ Creates, initializes, and starts a system instance in standalone mode without using a script. During initialization, system properties are read from a file specified on the command line.

(no prefix) System server application.

2. The basic name of the system (FTTCamSystem or FTTEnvSystem).

3. A suffix describing any network interface to the control GUI.

(no suffix) No control GUI interface.

_ucamcontrol Full control GUI interface; GSI interface spreadsheet excludes commands that change the system state.

_ucamdisplay Limited control GUI interface that does not allow clients to change the system-state.

Each interface spreadsheet defines a unique name for the system, comprising the last two components of the executable filename.

The particular variants that will be implemented are summarised in Table 2. Note that test executables are not installed by `make install`. The `ucamdisplay` spreadsheet differs from the base “no suffix” spreadsheet by the addition of a command to start the (limited) GUI interface. The `ucamcontrol` spreadsheet omits all of the state change commands of the base system, and adds a command to start the GUI interface. The three spreadsheets also use different names for the system as mentioned above. In all other respects the spreadsheets are identical for the three variants.

Executable	Spreadsheet (.ods)	Description
utest_FTT[X]System	FTT[X]System	Standalone unit test by direct method calls
FTT[X]System	FTT[X]System	System server without control GUI interface
utest_FTT[X]System_ucamcontrol	FTT[X]System_ucamcontrol	Standalone unit test via control GUI interface
start_FTT[X]System_ucamcontrol	FTT[X]System_ucamcontrol	Standalone with control GUI interface
FTT[X]System_ucamcontrol	FTT[X]System_ucamcontrol	System server with control GUI interface
start_FTT[X]System_ucamdisplay	FTT[X]System_ucamdisplay	Standalone with display-only GUI interface
FTT[X]System_ucamdisplay	FTT[X]System_ucamdisplay	System server with display-only GUI interface

Table 2: System variants. Each entry in the table describes a pair of systems, the system controller *FTTCamSystem* and the environment controller *FTTEnvSystem*.

3.1.1 C Implementation

The need to have several alternative system names for *FTTCamSystem* and *FTTEnvSystem* introduces a number of difficulties for sharing code between variants in the C implementation. In brief, the following differences between C code generated from different spreadsheets must be accommodated:

- The generated source files have different filenames.
- The C names of the system object differ.
- The state change action methods have different names (e.g. `initializeFTTCamSystem_ucamdisplayAction()`) (because the method names incorporate the system name).

Our solution to these difficulties involves post-processing the generated C code, the steps being as follows:

1. Generate C header and source files for the server and Java source for the client from the interface spreadsheet (e.g. `FTTCamSystem_ucamcontrol.ods` with system name “`FTTCamSystem_ucamcontrol`”).
2. Perform a global replacement of the system name from the spreadsheet (e.g. “`FTTCamSystem_ucamcontrol`”) with “`FTTCamSystem`” in the generated C header and source files. The Java client source is not modified.
3. Rename the C header and source files to `FTTCamSystem.h` and `FTTCamSystemInterface.c`.
4. Use the post-processed C header and source files to build the executables for that spreadsheet.
5. Repeat the process for the next spreadsheet, overwriting the previous post-processed C header and source files with new ones.

The post-processing described above is more or less equivalent to using a common system name for all variants on the server side, but different ones on the client side according to the spreadsheet used. The code-generation could in principle be modified to avoid the need for this post-processing.

A further issue is that the `ucamcontrol` variants omit the state-change commands from their spreadsheet, but prototypes for these command methods are still needed to build the `DLMsg` interface. We deal with this by introducing a (non-generated) header file `FTTCamSystemIncludes.h` containing the required declarations.

4 Interface Control

The GSI interfaces are defined precisely in the interface definition spreadsheets. The following is a summary of the interfaces for the system controller and the environment controller.

4.1 System controller interface

Some context is helpful for understanding the system controller interface. When the system is in the standard “Operational” state it can operate in any of three modes:

1. Idle. The camera is not reading out images, but commands are still accepted and monitor points are published once the relevant commands (`startPublish` and `startUcamControl` or `startUcamDisplay` have been received.
2. Acquisition. The camera is reading out full frame images using the manufacturer’s conventional clocking scheme. This state is intended for acquisition of celestial objects – that is, getting an object image onto the correct CCD pixels so that the fast tip-tilt mode can be activated.
3. Fast tip-tilt. The camera is continuously reading out a subframe defined when entering this mode. The readout can use the manufacturer’s conventional clocking scheme, or a customised scheme optimised for speed. This state is intended to acquire images with sufficient speed to close the servo loop.

4.1.1 System properties

The system properties are configuration values set up when the program is started, either by the ISS if available or via the GSI stand-alone execution environment if it is not. They are not expected to change during execution, unless specifically stated. All of these properties will be stored as string data types in the central configuration database.

University of Cambridge dlmsg interface These parameters define system connections from the Cambridge University control GUI and to the environment controller when the dlmsg interface is used.

- **UcamSysCmdPort** Command server port number, to accept commands from the control GUI. The control GUI “SupervisorPort” configuration parameter must match.
- **UcamSysDataPort** Data server port number, to send data to the control GUI. The control GUI “ServerPort” configuration parameter must match.
- **UcamConnectToEnv** Boolean (“true” or “false”). When true, the system will connect to the environment controller and watch its *CameraEnable* monitor point. If that value should become false, the system will commence an orderly shutdown.
- **UcamEnvIpAddr** The Internet Protocol address of the environment controller. It is prudent to use a numerical address in case no name server is available (for example, during network failure outside the control rack).
- **UcamEnvDataPort** Environment controller data server port number; value must match FTTEnvSystem property `UcamEnvDataPort`.

Emulation The system can be configured to work if either the analogue input/output card or the EMCCD camera are not present.

- **UseIOCard** Boolean (“true” or “false”). Enable/disable the interface to the FTTA. (Value ignored if using FLC command subset).
- **UseCamera** Boolean (“true” or “false”). Enable/disable use of the real camera (otherwise an internal simulation is used).

Electron multiplying gain These are either preset limits on allowed electron multiplying gain, or preset values that can be used to acquire standardised data.

- **MinEMGain** Minimum allowed electron multiplying gain.
- **MaxEMGain** Maximum allowed electron multiplying gain.
- **LowEMGain** Standardised low electron multiplying gain.
- **HighEMGain** Standardised high electron multiplying gain.

Exposure time These values are either preset limits on allowed exposure time, or preset values that can be used to acquire standardised data.

- **MinExpTime** Minimum allowed exposure time.
- **MaxExpTime** Maximum allowed exposure time.
- **AvgFullFrameExpTime** Exposure time used to acquire full frames for averaging (see [getAvgFrame](#)).
- **AvgConvenSubFrameExpTime** Exposure time used to acquire conventional readout subframes for averaging (see [getAvgFrame](#)). (Value ignored if using FLC command subset).
- **AvgCustomSubFrameExpTime** Exposure time used to acquire custom readout subframes for averaging (see [getAvgFrame](#)). (Value ignored if using FLC command subset).
- **DarkFullFrameExpTime** Exposure time used to acquire dark full frames for averaging (see [getDarkFrame](#) and [getSkyFrame](#)).
- **DarkConvenSubFrameExpTime** Exposure time used to acquire conventional readout dark subframes for averaging (see [getDarkFrame](#) and [getSkyFrame](#)). (Value ignored if using FLC command subset).
- **DarkCustomSubFrameExpTime** Exposure time used to acquire custom readout dark subframes for averaging (see [getDarkFrame](#) and [getSkyFrame](#)). (Value ignored if using FLC command subset).
- **FlatExpTime** Exposure time used to acquire flat fields for averaging (see [getFlatField](#)).

Clock induced charge These parameters describe the EMCCD clock induced charge pattern noise. Parameters may vary between cameras or as a camera ages.

- **CICPerParallelClock** Average clock induced charge per pixel per parallel clock, in electrons. Used to calculate Kalman filter measurement variance. (Value ignored if using FLC command subset).
- **CustomNBin** Number of pixels binned together in custom readout. Used to calculate Kalman filter measurement variance. (Value ignored if using FLC command subset).

Periods Limits on camera readout period in acquisition and fast tip-tilt mode.

- **MinAcquirePeriod** Minimum allowed frame period in acquisition mode.
- **MaxAcquirePeriod** Maximum allowed frame period in acquisition mode.
- **MinTipTiltPeriod** Minimum allowed frame period in fast tip-tilt mode. (Value ignored if using FLC command subset).
- **MaxTipTiltPeriod** Maximum allowed frame period in fast tip-tilt mode. (Value ignored if using FLC command subset).

Acquisition tolerance Some commands transition automatically between acquisition and fast tip-tilt or idle mode when an object is acquired. These parameters determine when the change is made.

- **AcquireTolerance** Threshold that determines when an object is considered to be acquired.
- **AcquireFrameAvg** Number of frames to average when calculating AcquireTolerance.

Hardware constants These values are intrinsic to the camera hardware and the optics. They are needed for calculating the pixel scale and field size.

- **MaxPixelValue** Maximum pixel value allowed by the camera hardware.
- **PixelSize** Length of the edge of each pixel.
- **DetectorWidth** Width of the sensitive area of the CCD.
- **DetectorHeight** Height of the sensitive area of the CCD.
- **CameraFocalLength** Focal length of the local fast tip-tilt lens.
- **OpticalGainX** Factor to account for optical geometry and reflections in X axis.
- **OpticalGainY** Factor to account for optical geometry and reflections in Y axis.
- **UTMagnification** Magnification of the unit telescope.
- **UTDiameter** Diameter of the unit telescope aperture. (Value ignored if using FLC command subset).
- **TipTiltResponse** Scaling factor between FTTA angle and applied voltage. (Value ignored if using FLC command subset).
- **Nas0** A calibrated constant that describes the rotation between the pixel frame and the azimuth/elevation frame.
- **AllowAuxTipTiltIn** Boolean (“true” or “false”). Enable/disable reading and publishing of auxiliary tip/tilt voltages *AuxTip* and *AuxTilt*. These signals are used for closed-loop testing. (Value ignored if using FLC command subset).
- **CameraAirCooling** Boolean (“true” or “false”). Enable/disable use of the camera’s internal fan for cooling. Enable this if an external chilled fluid supply is not available.
- **CCDSetTemp** The desired temperature set-point for the EMCCD camera.

Tip-tilt camera readout These values determine the size of the readout square in fast tip-tilt mode for the different clocking schemes, and whether the custom clocking scheme may be used.

- **CustomTipTiltSquareWidth** Width in pixels of the square used with the custom clocking scheme in fast tip-tilt mode. (Value ignored if using FLC command subset).

- **ConvenTipTiltSquareWidth** Width in pixels of the square used with the conventional clocking scheme in fast tip-tilt mode. (Value ignored if using FLC command subset).
- **AllowCustomReadout** Boolean (“true” or “false”). True to permit use of the custom clocking scheme. (Value ignored if using FLC command subset).

Tip-tilt servo parameters These parameters determine the behaviour of the tip-tilt servo if Kalman filtering is disabled.

- **DefaultTipTiltBandwidth** Default bandwidth of tip-tilt servo. (Value ignored if using FLC command subset).
- **MaxServoGain** Ceiling on gain selected by **setTipTiltBandwidth**. (Value ignored if using FLC command subset).

Kalman filter parameters These parameters are used to calculate the Kalman filter variance parameters (see **setAutoKalmanProcessVar** and **setAutoKalmanMeasureVar** commands) for fast tip-tilt mode.

- **DefaultKalmanErrorEst** Default Kalman filter initial error estimate, used before the system has completed a fast tip-tilt mode run. (Value ignored if using FLC command subset).
- **DefaultWindDir** Default seeing wind speed, used before the system has completed a fast tip-tilt mode run. (Value ignored if using FLC command subset).
- **DefaultWindVel** Default seeing wind direction, used before the system has completed a fast tip-tilt mode run. (Value ignored if using FLC command subset).
- **DefaultFriedParam** Default r_0 , used before the system has completed a fast tip-tilt mode run. (Value ignored if using FLC command subset).
- **DefaultPhotonRate** Default detected photon rate from reference object, used before the system has completed a fast tip-tilt mode run. (Value ignored if using FLC command subset).
- **OuterScale** Outer scale of turbulence. (Value ignored if using FLC command subset).
- **EffectiveWavelength** Effective wavelength of UT/FTT optics and detector. (Value ignored if using FLC command subset).

Seeing estimation These are the parameters used to estimate the seeing and related parameters from image data.

- **SeeingAvgTime** Time over which *AvgSeeingFWHM* and *AvgPhotonRate* monitor points are calculated.

Offload period This is the (reciprocal of the) maximum rate at which UTM offloads are sent to the telescope.

- **OffloadPeriod** Period of UTM offloads sent

4.1.2 Control

Commands can be broadly divided into three categories:

- Configuration modifiers. These commands modify the configuration of the system controller.
- Readout commands. These commands initiate camera readout in either acquisition or fast tip-tilt modes. Some continue camera readout until told to stop, others progress through a preset sequence of readout tasks.

- Information requests. These commands return information about the system settings or tell the system to start publishing to the ISS or to subscribe to the environment controller “cameraEnable” monitor point.

The commands themselves are as follows:

University of Cambridge control GUI interface These commands enable the communications interface with the Cambridge control GUI.

- **startUcamControl** Enable full control via University of Cambridge dlmsg protocol. (Only available in ucamcontrol variants).
- **startUcamDisplay** Enable viewing via University of Cambridge dlmsg protocol, with no state changes allowed. (Only available in ucamdisplay variants).

Configuration modifiers These commands modify the configuration of the system controller.

Electron multiplying gain These commands can be called in any mode. They modify the electron multiplication gain setting of the camera.

- **setEMGain** Set electron multiplying gain to specified value.
- **setToLowEMGain** Set electron multiplying gain to the LowEMGain preset value.
- **setToHighEMGain** Set electron multiplying gain to the HighEMGain preset value.

Tube offset These commands can be called in any mode. They tell the system controller whether the local telescope is in tube offset mode or not. This information is needed to calculate the camera pixel scale.

- **setTubeOffsetOn** Inform the system that the telescope is in tube offset mode.
- **setTubeOffsetOff** Inform the system that the telescope is not in tube offset mode.

Zero point This command can be called in any mode. It sets the target image position on the EMCCD.

- **setTipTiltZeroPoint** Set the target position (in EMCCD pixel coordinates, prior to application of telescope dispersion and off-axis offsets) for acquisition and fast tip-tilt.

Reference object selection These commands work in acquisition mode. They select the “reference object”, the image of the celestial object to be acquired, which may not be the science target.

- **setAcquireScopeRect** Set reference object to brightest object within predefined rectangle.
- **setAcquireScopeField** Set reference object to brightest object in entire field.
- **unsetAcquireScope** Unset reference object.

Camera frame timing These commands set the camera frame timing to be used in acquisition mode or fast tip-tilt mode. There is no command to set the exposure time in fast tip-tilt mode, it is always set to the maximum compatible with the period.

- **setAcquirePeriod** Set the time between EMCCD acquisition frames.
- **setAcquireExpTime** Set exposure time for each acquisition frame.

- **setTipTiltPeriod** Set the time between fast tip-tilt frames. (Not in FLC command subset).

Decimation Decimation is a method of reducing network bandwidth and storage requirements. If the decimation is n , then only one camera frame in every n is published. Other data taken at the camera frame rate are bundled together so that n frames' worth are published at the same time. Hence there is one image published for every bundle published.

- **setAcquireDecimation** Set the decimation n for acquisition frames.
- **setTipTiltDecimation** Set the decimation n for fast tip-tilt frames. (Not in FLC command subset).

Clocking In fast tip-tilt mode the readout can use the manufacturer's conventional clocking scheme, or a customised scheme optimised for speed.

- **setTipTiltCustomReadout** Use custom clocking scheme for fast tip-tilt readout. (Not in FLC command subset).
- **setTipTiltConvenReadout** Use conventional clocking scheme for fast tip-tilt readout. (Not in FLC command subset).

Servo parameters In fast tip-tilt mode, a servo can be used to stabilise the target image position on the EMCCD through actuation of the fast tip-tilt mirror. These commands control the servo behaviour.

- **setTipTiltLoopOpen** Open the fast tip-tilt servo loop. (Not in FLC command subset).
- **setTipTiltLoopClosed** Close the fast tip-tilt servo loop. (Not in FLC command subset).
- **setTipTiltServoGain** Explicitly set closed loop servo gain. (Not in FLC command subset).
- **setTipTiltBandwidth** Set closed loop bandwidth by adjusting frame period and servo gain. Possibly also chooses between conventional and custom clocking scheme. (Not in FLC command subset).
- **kalmanFilterOn** Turn on adaptive servo filter. (Not in FLC command subset).
- **kalmanFilterOff** Turn off adaptive servo filter. (Not in FLC command subset).
- **setAutoKalmanProcessVar** Use seeing estimates to calculate Kalman filter process variance. (Not in FLC command subset).
- **setAutoKalmanMeasureVar** Use photon rate estimates to calculate Kalman filter measurement variance (Not in FLC command subset).
- **setKalmanProcessVar** Set Kalman filter process variance to specified value (Not in FLC command subset).
- **setKalmanMeasureVar** Set Kalman filter measurement variance to specified value (Not in FLC command subset).

Background subtraction These commands control the use of previously acquired or generated images to de-bias the centroids calculated from the pixel data. The system stores separate dark frames for each of three frame types: full frames, conventional readout subframes, and custom readout subframes.

- **setDarkFrame** Use the provided image for dark subtraction when capturing the specified frame type. The integer-typed first parameter specifies the frame type: 0 = full frame; 1 = conventional readout subframe; 2 = custom readout subframe. The latter two frame types are not relevant to the FLC command subset.
- **unsetDarkFrame** Do not do dark subtraction for the specified frame type.
- **setFlatField** Use the provided image for flat field correction.
- **unsetFlatField** Do not do flat field correction.

Readout commands These commands initiate or stop camera readout in either acquisition or fast tip-tilt modes. Some continue camera readout until told to stop, others progress through a preset sequence of readout tasks.

Observational readout These commands are intended for use in acquiring objects and then stabilising their images while science observations are made.

- **startAcquireRun** Change to acquisition mode and read out full frame continuously.
- **getObject** Change to acquisition mode, acquire and return when object is acquired.
- **acquireAndGuide** Change to acquisition mode and acquire until **stopRun** is called.
- **acquireAndStartTipTiltRun** Change to acquisition mode, acquire object, then change to fast tip-tilt mode with servo closed. (Not in FLC command subset).
- **startTipTiltRun** Change to fast tip-tilt mode with servo closed. (Not in FLC command subset).
- **startTipTiltRunNoServo** Change to fast tip-tilt mode with servo open. (Not in FLC command subset).
- **stopRun** Stop any ongoing readout.

Background subtraction These commands acquire sets of images and average them. The images can be used later to de-bias centroids calculated during readout. The system properties specify a total of seven standardised exposure times: two exposure times (for average frames and dark/sky frames) for each of three frame types (full frame, conventional readout subframe, custom readout subframe) as well an exposure time for flat fields (which are always full frames).

- **getAvgFrame** Returns a standardised camera frame of the specified type (0 = full frame; 1 = conventional readout subframe; 2 = custom readout subframe) that is an average of the specified number of frames.
- **getDarkFrame** Like **getAvgFrame** but with the camera shutter closed.
- **getSkyFrame** Like **getAvgFrame** but taken on the sky.
- **getFlatField** Like **getAvgFrame** but taken against an (assumed) uniformly illuminated field.

Information requests These commands return information about the system settings or current state, or tell the system to start publishing to the ISS or to subscribe to the environment controller “cameraEnable” monitor point.

- **getFixedParams** Retrieve settings that are constant over the program run time.

- **startPublish** Start publishing monitor points (DLMsg messaging is not affected).
- **startSubscribe** Subscribe to the environment controller's "cameraEnable" monitor point.

4.1.3 Monitor points

Monitor points for the system controller can most conveniently be grouped by frequency of generation. Note that several combinations of these groups can be being published, depending on the state of the system.

Information about the status of the system controller is sent at a rate that gives "instant" feedback on a human timescale (currently set to 10 Hz). Monitor points in this category include:

TubeOffsetMode Boolean. True if the system has been told the telescope is in tube offset mode.

CameraReadout Boolean. True if the camera is reading out.

ShutterOpen Boolean. True if the shutter is open.

CameraTemp Floating point. The camera CCD chip temperature.

ExpTime Floating point. The current exposure time.

EMGain Integer. The electron multiplying gain, on an arbitrary scale set by Andor.

AcquirePeriod Floating point. The time between frames to be used in acquisition mode.

AcquireExpTime Floating point. The duration of exposures to be used in acquisition mode.

AcquireReadoutTime Floating point. The time required to read out an image in acquisition mode.

AcquireMaxExpForPeriod Floating point. Maximum possible exposure time available for *AcquirePeriod*.

AcquireDecimation Integer. The decimation rate, used to reduce the number of acquisition mode images sent.

TipTiltPeriod Floating point. The time between frames to be used in fast tip-tilt mode. (Not relevant to FLC command subset).

TipTiltExpTime Floating point. The duration of exposures to be used in fast tip-tilt mode. (Not relevant to FLC command subset).

TipTiltReadoutTime Floating point. The time required to read out an image in fast tip-tilt mode. (Not relevant to FLC command subset).

TipTiltDecimation Integer. The decimation rate, used to reduce the number of fast tip-tilt mode images sent and to determine how much high bandwidth data should be chunked together before it is sent. (Not relevant to FLC command subset).

ReadoutSquareX Integer. X pixel coordinate of fast tip-tilt square readout region. (Not relevant to FLC command subset).

ReadoutSquareY Integer. Y pixel coordinate of fast tip-tilt square readout region. (Not relevant to FLC command subset).

AcquireRectX Integer. X pixel coordinate of acquisition rectangle.

AcquireRectY Integer. Y pixel coordinate of acquisition rectangle.

- AcquireRectWidth*** Integer. Pixel width of acquisition rectangle.
- AcquireRectHeight*** Integer. Pixel height of acquisition rectangle.
- OffloadGain*** Floating point. Multiplier for telescope offload values prior to being sent for telescope correction.
- TipTiltZeroPointX*** Floating point. X pixel coordinate of target closed loop servo position, prior to application of telescope dispersion and off-axis offsets.
- TipTiltZeroPointY*** Floating point. Y pixel coordinate of target closed loop servo position, prior to application of telescope dispersion and off-axis offsets.
- ObjectivePointX*** Floating point. X pixel coordinate of target position, after application of telescope dispersion and off-axis offsets.
- ObjectivePointY*** Floating point. Y pixel coordinate of target position, after application of telescope dispersion and off-axis offsets.
- RotG11*** Floating point. Element G_{11} of the rotation matrix that converts from CCD axes to tip-tilt mirror axes. This depends on the telescope pointing. (Not relevant to FLC command subset).
- RotG12*** Floating point. Element G_{12} of the rotation matrix. (Not relevant to FLC command subset).
- RotG21*** Floating point. Element G_{21} of the rotation matrix. (Not relevant to FLC command subset).
- RotG22*** Floating point. Element G_{22} of the rotation matrix. (Not relevant to FLC command subset).
- RotT11*** Floating point. Element T_{11} of the rotation matrix that converts between Nasmyth and RA/Dec coordinates. This depends on the telescope pointing.
- RotT12*** Floating point. Element T_{12} of the rotation matrix.
- RotT21*** Floating point. Element T_{21} of the rotation matrix.
- RotT22*** Floating point. Element T_{22} of the rotation matrix.
- AcquireScopeSet*** Boolean. True if acquisition scope is set.
- AcquireActive*** Boolean. True if acquisition mode is active
- FastTipTiltActive*** Boolean. True if fast tip-tilt mode is active. (Not relevant to FLC command subset).
- GettingObject*** Boolean. True if the **getObject** command is executing.
- AcquiringAvg*** Boolean. True if the system is in the process of acquiring data for an average frame.
- AcquiringDarkAvg*** Boolean. True if the system is in the process of acquiring data for a dark average frame.
- AcquiringSkyAvg*** Boolean. True if the system is in the process of acquiring data for a sky average frame.
- AcquiringFlatAvg*** Boolean. True if the system is in the process of acquiring data for a flat field.
- GuidingObject*** Boolean. True if the system is in acquisition mode, has successfully acquired an object, and is continuing to keep it acquired.
- RunUntilStopped*** Boolean. True if executing a (synchronous) command that causes the camera to read out indefinitely, such as **startAcquireRun**.

TipTiltPending Boolean. True if executing a command that will eventually cause the system to change to fast tip-tilt mode (currently only **acquireAndStartTipTiltRun**). (Not relevant to FLC command subset).

GuidePending Boolean. True if executing a command that will eventually cause the system to guide in acquisition mode (currently only **acquireAndGuide**).

DarkFullFrameSet Boolean. True if a dark frame (which could be a sky frame) is being used to do dark subtraction for full frames.

DarkConvenSubFrameSet Boolean. True if a dark frame (which could be a sky frame) is being used to do dark subtraction for conventional readout subframes. (Not relevant to FLC command subset).

DarkCustomSubFrameSet Boolean. True if a dark frame (which could be a sky frame) is being used to do dark subtraction for custom readout subframes. (Not relevant to FLC command subset).

FlatFieldSet Boolean. True if a flat field is being used to do flat field corrections.

TipTiltServoGain Floating point. The current servo gain setting. (Not relevant to FLC command subset).

TipTiltBandwidth Floating point. The current fast tip-tilt loop bandwidth. (Not relevant to FLC command subset).

TipTiltLoopClosed Boolean. True if the fast tip-tilt loop is closed. (Not relevant to FLC command subset).

TipTiltCustomReadout Boolean. True if the custom clocking scheme is currently used to read out CCD images in fast tip-tilt mode. (Not relevant to FLC command subset).

KalmanFilterOn Boolean. True if the Kalman adaptive filter is on. (Not relevant to FLC command subset).

KalmanBandwidth Floating point. Servo bandwidth for current Kalman filter parameters. (Not relevant to FLC command subset).

KalmanProcessVar Floating point. The current Kalman filter process variance. (Not relevant to FLC command subset).

KalmanMeasureVar Floating point. The current Kalman filter measurement variance. (Not relevant to FLC command subset).

AutoKalmanProcessVar Boolean. True if the Kalman filter process variance is being calculated automatically. (Not relevant to FLC command subset).

AutoKalmanMeasureVar Boolean. True if the Kalman filter measurement variance is being calculated automatically. (Not relevant to FLC command subset).

High bandwidth data is sampled at the current camera frame rate, which is expected to be as high as 1 kHz. If the current decimation rate is n , then data from every n frames is chunked together into time series prior to publication to improve the network efficiency. The exception is the camera images themselves, only one in every n is published to save bandwidth and storage. If the system is idle, none of this information is published.

High bandwidth monitor points include:

CentroidPixX Floating point time series. X coordinate of calculated image centroid.

CentroidPixY Floating point time series. Y coordinate of calculated image centroid.

KalmanCentroidPixX Floating point time series. Kalman estimate of centroid X coordinate. (Not relevant to FLC command subset).

KalmanCentroidPixY Floating point time series. Kalman estimate of centroid Y coordinate. (Not relevant to FLC command subset).

ResidualCentroidPixX Floating point time series. Centroid X coordinate with mirror tip/tilt removed (Not relevant to FLC command subset).

ResidualCentroidPixY Floating point time series. Centroid Y coordinate with mirror tip/tilt removed (Not relevant to FLC command subset).

KalmanGainX Floating point time series. Current Kalman adaptive filter X gain. (Not relevant to FLC command subset).

KalmanGainY Floating point time series. Current Kalman adaptive filter Y gain. (Not relevant to FLC command subset).

CentroidValid Boolean time series. True if the system thinks that the calculated centroid value is valid.

OffsetX Floating point time series. The X angle between the current centroid and the target position.

OffsetY Floating point time series. The Y angle between the current centroid and the target position.

MirrorTipDemand Floating point time series. The voltage being sent to the mirror tip axis. (Not relevant to FLC command subset).

MirrorTiltDemand Floating point time series. The voltage being sent to the mirror tilt axis. (Not relevant to FLC command subset).

MirrorTip Floating point time series. The mirror tip axis position. (Not relevant to FLC command subset).

MirrorTilt Floating point time series. The mirror tilt axis position. (Not relevant to FLC command subset).

AuxTip Floating point time series. Auxiliary tip voltage readback (only published automatically if [AllowAuxTipTiltIn](#) is set to true). (Not relevant to FLC command subset).

AuxTilt Floating point time series. Auxiliary tilt voltage readback (only published automatically if [AllowAuxTipTiltIn](#) is set to true). (Not relevant to FLC command subset).

InstantSeeingFWHM Floating point. Spatial seeing estimate (expressed as a conventional long exposure image FWHM) from the latest frame.

InstantSeeingErr Floating point. Estimated error in *InstantSeeingFWHM*.

AvgSeeingFWHM Floating point. Spatial seeing averaged over [SeeingAvgTime](#).

AvgSeeingErr Floating point. Estimated error in *AvgSeeingFWHM*.

AvgCentroidErr Floating point. RMS distance of the centroid from the tip-tilt zero point.

CoherenceTime Floating point. Estimate of the coherence time (temporal seeing). (Not relevant to FLC command subset).

CoherenceTimeErr Floating point. Estimated error in *CoherenceTime*. (Not relevant to FLC command subset).

InstantPhotonRate Floating point. Detected photons/sec for the tip-tilt reference object from the latest frame.

AvgPhotonRate Floating point. Photon rate averaged over [SeeingAvgTime](#).

Frame Integer 2D array. Camera image.

Finally, telescope steering corrections (“offloads”) are published at the rate at which they are sent to the telescope, which is either a fixed rate (expected to be 1 Hz) or the camera frame rate if that is lower. The offload values and their timestamps must be supplied to the dedicated FTTA offload socket interface described in Sec. 8.11 of RD5. It is also MRO’s responsibility to configure this interface appropriately and to activate it prior to use of the target acquisition or fast tip-tilt modes of the FTT/NAS. We will provide details of how the offload interface should be configured in a later revision of this ICD. If the system is idle, none of this information is published.

The telescope steering correction monitor points are;

OffloadX Floating point. X value of UTM offload.

OffloadY Floating point. Y value of UTM offload.

4.1.4 Subscriptions

Subscriptions which the FTT/NAS must access from the UT via the publish subscribe system are listed below with a short description, the status word and either the matrix coefficient names or units in the case of a scalar value, as described in RD6.

- Telescope rotation matrix for conversion between Nasmyth and FTTA coordinates:
garray g00,g01,g10,g11
- Telescope rotation matrix for conversion between Nasmyth and RA/Dec coordinates:
tarray t00,t01,t10,t11
- Current focal plane ξ coordinate of the guide target
xi arcsecs
- Current focal plane η coordinate of the guide target
eta arcsecs
- Predicted focal plane ξ value for the guide target.
predictedxi arcsecs
- Predicted focal plane η value for the guide target.
predictedeta arcsecs
- Outer axis position
outer degs

The corrections that the FTT/NAS sends to the FTTA are initially derived in the detector coordinate frame and must be rotated and scaled appropriately to produce the correct tip and tilt displacements in the FTTA coordinate frame. For this calculation the rotation correction between the detector coordinate frame and the Nasmyth focal plane must be determined, and the rotation matrix between the Nasmyth focal plane and the FTTA coordinate frame must be known. The former requires the combination of the [Nas0](#) parameter (available from the FTT/NAS system properties) and the outer axis position variable `outer` which must be subscribed to. The latter requires the rotation matrix `garray` to be subscribed to. To represent RA/DEC coordinates on user displays the rotation matrix for conversion between nasmyth and

RA/DEC, `tarray`, is also subscribed to. To ensure that correct values of the guide offset are generated, the ISS should command the UTCS in order to set the coordinates of the guide target (if using an off-axis tip-tilt reference, otherwise the guide target coordinates should be set as those of the science target) and the effective wavelengths of the FTT/NAS sensor and the appropriate beam combining instrument. To compute the position offset of the guide star in EMCCD pixel coordinates (for both the current guide star position and for the predicted position 300 seconds in the future) the focal plane ξ and η values are rotated to the detector coordinate frame using `outer` and `Nas0`, as described before. The FTT/NAS system properties `PixelSize`, `CameraFocalLength` and `UTMagnification` are then used to convert the result to pixels. The `Nas0`, `PixelSize`, `CameraFocalLength` and `UTMagnification` system properties must be consistent with their equivalents in the UTCS.

If the Cambridge University `dlmsg` interface is not in use, one subscription is required from the FTT/NAS environment controller:

- **CameraEnable** Boolean. True if the environment controller is allowing the camera to run.

4.1.5 Faults

CameraTooHot Shut down camera and program if the camera temperature gets too hot.

4.2 Environment controller interface

4.2.1 System properties

The system properties of the environment controller define software and hardware interfaces and the environmental conditions within which the camera has permission to operate.

University of Cambridge control GUI interface These parameters define the port numbers on which the system listens for connections from the the control GUI. The values must match the corresponding control GUI configuration parameters.

- **UcamEnvCmdPort** Command server port number.
- **UcamEnvDataPort** Data server port number.

LabJack interface These parameters identify each of the LabJacks used for analog and I²C interfacing, so they can be automatically identified when plugged into the host computer's USB ports.

- **UseInterface** Boolean (“true” or “false”). When true, the environment controller will use the Labjacks. Otherwise, software emulation is used.
- **LabJack1Id** Identifier (serial number on base) of LabJack “1” (closest to Raspberry Pi in chassis).
- **LabJack2Id** Identifier (serial number on base) of LabJack “2”.

Temperature Temperature conditions.

- **EnclosureAirMaxTemp** Maximum allowed air temperature within the camera enclosure.
- **EnclosureAirMinTemp** Minimum allowed air temperature within the camera enclosure.
- **EnclosureAirMinPassiveTemp** Minimum allowed air temperature within the camera enclosure for the camera to be enabled.

- **CoolantMaxBelowAmbient** The coolant entry temperature must be at least this close to the enclosure air temperature.
- **CoolantMinAboveDewPoint** The coolant entry temperature must be warmer than the dew point by this amount.
- **EnclosureSurfMaxAboveAmbient** The external enclosure surface must be less than this amount above the ambient temperature.
- **EnclosureSurfMaxBelowAmbient** The external enclosure surface must be less than this amount below the ambient temperature.
- **EnclosureSurfMaxPassiveBelowAmbient** The external enclosure surface must be less than this amount below the ambient temperature before the camera can be enabled.

Humidity Humidity conditions.

- **EnclosureMinHumidity** Minimum allowed humidity within the camera enclosure.
- **EnclosureMaxHumidity** Maximum allowed humidity within the camera enclosure.

Flow rate Flow rate conditions. These only produce warnings if the conditions are not met. The camera still has permission to operate.

- **MinCoolantFlow** The minimum coolant flow needed.
- **MinAirFlow** The minimum air flow needed.

Calibration Parameters used to improve sensor accuracy. For each listed sensor, the raw output is multiplied by the gain and an offset is added to the result. Hence the calibration is a simple linear remapping.

- **EnclosureAirTempGain** Enclosure air temperature gain adjustment.
- **EnclosureAirTempOffset** Enclosure air temperature offset adjustment.
- **EnclosureHumidityGain** Enclosure humidity gain adjustment.
- **EnclosureHumidityOffset** Enclosure humidity offset adjustment.
- **CoolantOutTempGain** Coolant exit temperature gain adjustment.
- **CoolantOutTempOffset** Coolant exit temperature offset adjustment.
- **CameraMountTempGain** Camera mount temperature gain adjustment.
- **CameraMountTempOffset** Camera mount temperature offset adjustment.
- **CameraCaseTempGain** Camera case temperature gain adjustment.
- **CameraCaseTempOffset** Camera case temperature offset adjustment.
- **CoolantInTempGain** Coolant entry temperature gain adjustment.
- **CoolantInTempOffset** Coolant entry temperature offset adjustment.
- **HeaterTempGain** Heater temperature gain adjustment.
- **HeaterTempOffset** Heater temperature offset adjustment.
- **EnclosureTableTempGain** Table temperature near enclosure gain adjustment.
- **EnclosureTableTempOffset** Table temperature near enclosure offset adjustment.

- **EnclosureSurfTempGain** Enclosure surface temperature gain adjustment.
- **EnclosureSurfTempOffset** Enclosure surface temperature offset adjustment.
- **EnclosureMountTempGain** Enclosure mount temperature gain adjustment.
- **EnclosureMountTempOffset** Enclosure mount temperature offset adjustment.
- **AmbientTempGain** Ambient temperature gain adjustment.
- **AmbientTempOffset** Ambient temperature offset adjustment.
- **AmbientHumidityGain** Ambient humidity gain adjustment.
- **AmbientHumidityOffset** Ambient humidity offset adjustment.
- **BaseplateTableTempGain** Table temperature near baseplate gain adjustment.
- **BaseplateTableTempOffset** Table temperature near baseplate offset adjustment.
- **BaseplateTemp1Gain** Baseplate temperature 1 gain adjustment.
- **BaseplateTemp1Offset** Baseplate temperature 1 offset adjustment.
- **BaseplateTemp2Gain** Baseplate temperature 2 gain adjustment.
- **BaseplateTemp2Offset** Baseplate temperature 2 offset adjustment.
- **BaseplateTemp3Gain** Baseplate temperature 3 gain adjustment.
- **BaseplateTemp3Offset** Baseplate temperature 3 offset adjustment.
- **BaseplateTemp4Gain** Baseplate temperature 4 gain adjustment.
- **BaseplateTemp4Offset** Baseplate temperature 4 offset adjustment.
- **BaseplateTemp5Gain** Baseplate temperature 5 gain adjustment.
- **BaseplateTemp5Offset** Baseplate temperature 5 offset adjustment.
- **BaseplateTemp6Gain** Baseplate temperature 6 gain adjustment.
- **BaseplateTemp6Offset** Baseplate temperature 6 offset adjustment.
- **BaseplateTemp7Gain** Baseplate temperature 7 gain adjustment.
- **BaseplateTemp7Offset** Baseplate temperature 7 offset adjustment.
- **CoolantFlowGain** Coolant flow rate gain adjustment.
- **CoolantFlowOffset** Coolant flow rate offset adjustment.
- **AirFlowGain** Dry air flow rate gain adjustment.
- **AirFlowOffset** Dry air flow rate offset adjustment.

Shutdown and power outlet control Parameters that affect how the environment controller shuts down the FTT/NAS system, including removal of power to the camera and the FTT/NAS computer.

- **FTTShutdownEnable** Boolean (“true” or “false”). When true, the environment controller is permitted to shutdown the camera system software and the FTT/NAS computer.

- **FTTPowerControlEnable** Boolean (“true” or “false”). When true, the environment controller is permitted to use the ethernet-switched mains power board within the control rack to cut the power to the camera and the FTT/NAS computer.
- **FTTShutdownSeconds** The time between detection of an adverse environmental condition and shutdown of the camera system software and the FTT/NAS computer.
- **FTTPowerdownSeconds** If **FTTPowerControlEnable** is true, this is the time from the end of the **FTTShutdownSeconds** countdown until the mains power is removed from the camera and the FTT/NAS computer.
- **FTTShutdownUser** The username and internet protocol address of the user on the FTT/NAS computer whose account is used to initiate a shutdown of that computer.
- **FTTPowerIPAddr** The internet protocol address of the ethernet-switched power board.
- **FTTPowerIPPort** The internet protocol port of the ethernet-switched power board.
- **FTTPowerLogin** The string used to log in to the ethernet-switched power board.
- **FTTPowerComputerOutletNumber** The outlet number on the ethernet-switched power board that supplies power to the FTT/NAS computer.
- **FTTPowerCameraOutletNumber** The outlet number on the ethernet-switched power board that supplies power to the camera Peltier cooler.

4.2.2 Control

The environment controller has only one operational state, in which it publishes environment measurements, (optionally) controls a heater in the camera enclosure and (optionally) enables or disables camera operation. The command set is as follows:

University of Cambridge control GUI interface These commands enable the communications interface with the Cambridge control GUI.

- **startUcamControl** Enable full control via University of Cambridge dlmsg protocol. (Only available in ucamcontrol variants).
- **startUcamDisplay** Enable viewing via University of Cambridge dlmsg protocol, with no state changes allowed. (Only available in ucamdisplay variants).

Heater commands These commands control the camera enclosure heater or allow it to work automatically.

- **setHeatAuto** Allow the environment controller to control the heater state automatically.
- **setHeatManual** Control the heater manually.
- **setHeatOn** When manual heater control is enabled, turn the heater on.
- **setHeatOff** When manual heater control is enabled, turn the heater off.

Camera control commands These commands control whether the system controller uses the camera, or allow the environment controller to do so.

- **setCameraAuto** Allow the environment controller to shut down the FTT/NAS if it detects adverse environmental conditions.

- **setCameraManual** Allow manual camera shutdown. Cancels any shutdown countdown initiated in auto mode.
- **setCameraDisable** When manual camera control is on, initiate the FTT/NAS shutdown procedure.

Air flow control commands These commands activate the solenoid valve that turns the flow of dry air on or off.

- **setAirFlowOn** Turn on air flow to the camera enclosure.
- **setAirFlowOff** Turn off air flow to the camera enclosure.

Information requests These commands retrieve the environment controller fixed parameters or start publishing.

- **getFixedParams** Retrieve settings that are constant over the program run time.
- **startPublish** Start publishing monitor data to the ISS (this does not affect DLMsg messages).

4.2.3 Monitor points

The Generic System Interface monitor points for the environment controller generate scalars, booleans and Durations at a constant frequency, expected to be 1 Hz. The majority of these are environment data but there are a few status monitor points too. Environment controller monitor points include:

EnclosureAirTemp Floating Point. Air temperature inside the camera enclosure.

EnclosureAirHumidity Floating Point. Humidity inside the camera enclosure.

EnclosureAirDewPoint Floating Point. Calculated dew point inside the camera enclosure.

CoolantOutTemp Floating Point. Temperature of coolant as it exits the camera enclosure.

CoolantInTemp Floating Point. Temperature of coolant prior to entering the camera enclosure.

CameraCaseTemp Floating Point. Temperature of the camera case.

HeaterTemp Floating Point. Temperature of the heater inside the camera enclosure.

CameraMountTemp Floating Point. Temperature of the camera mount.

EnclosureTableTemp Floating Point. Temperature of the optical table near the enclosure.

EnclosureSurfTemp Floating Point. Temperature of the external enclosure surface.

EnclosureMountTemp Floating Point. Temperature of the external enclosure mount.

CoolantFlowRate Floating Point. Coolant flow rate.

AirFlowRate Floating Point. Flow rate of dry air blown onto the camera window.

LabJack1Temp Floating Point. Internal temperature of LabJack1.

AmbientTemp Floating Point. Air temperature outside the camera enclosure.

AmbientHumidity Floating Point. Humidity outside the camera enclosure.

AmbientDewPoint Floating Point. Dew point outside the camera enclosure.

BaseplateTableTemp Floating Point. Temperature of the optical table near the baseplate.

BaseplateTemp1 Floating Point. Baseplate temperature1.

BaseplateTemp2 Floating Point. Baseplate temperature2.

BaseplateTemp3 Floating Point. Baseplate temperature3.

BaseplateTemp4 Floating Point. Baseplate temperature4.

BaseplateTemp5 Floating Point. Baseplate temperature5.

BaseplateTemp6 Floating Point. Baseplate temperature6.

BaseplateTemp7 Floating Point. Baseplate temperature7.

LabJack2Temp Floating Point. Internal temperature of LabJack2.

HeaterAuto Boolean. True if the heater is being controlled by the application.

HeaterOn Boolean. True if the heater is on.

AirFlowOn Boolean. True if air flow to the camera enclosure is on.

CameraAuto Boolean. True if the camera enable is being controlled by the application.

CameraEnable Boolean. True if the environment controller is allowing the camera to run.

PowerControl Boolean. True if the environment controller has established control of the ethernet-switched power board.

ShutdownPending Boolean. The environment controller has detected an adverse environmental condition and has initiated the shutdown countdown.

PowerdownPending Boolean. The FTT/NAS shutdown is complete and the powerdown countdown is underway.

TimeToShutdown Duration. The time until the FTT/NAS is shut down.

TimeToPowerdown Duration. The time until power to the FTT/NAS computer and camera is cut.

ComputerPowerOn Boolean. Is the FTT/NAS computer power on?

CameraPowerOn Boolean. Is the camera power on?

4.2.4 Subscriptions

No subscriptions.

4.2.5 Faults

EnclosureTooHot Warn if enclosure is too hot.

EnclosureTooCold Warn if enclosure is too cold.

EnclosureTooDry Warn if enclosure is too dry.

EnclosureTooHumid Warn if enclosure is too humid.

Condensation Warn if coolant temperature is below dew point.

Coolant Warn if coolant temperature is more than 5 degrees below ambient.

CoolantFlowTooLow Warn if coolant flow is too low.

AirFlowTooLow Warn if air flow is too low. This fault is only enabled if the air flow is on and has been on for a fixed period of time (currently five seconds). This is to prevent warnings when the air flow valve is shut, and when the air flow valve has just been opened (before the air has reached the air flow sensor).

AirFlowValveFault The air flow valve driver is signaling a fault, which could be driver overheating or overcurrent or undercurrent.

HeaterControlFailed Warn if an error occurred when switching the heater on or off.

PowerInterfaceFailed Warn if an error occurred when querying or setting the state of an ethernet-switched power outlet.